

FIROUZI CONSULTING ENGINEER, INC.

SKYTRON SURGICAL PRODUCTS

DES.

SHEET

LFSst232323

FOR SEISMIC ZONE (4), SOIL PROFILE (Sd)
NEAR SOURCE FACTOR = 1.5

FCE
JOB No.

DATE: 4-6-04

1



OF 4 SHEETS

SEISMIC ANCHORING BOLT DESIGN

LFSst232323

***BY OTHERS:**

EQUIPMENT STRUCTURE SUPPORT AND
BRACING IS OUTSIDE SCOPE OF THIS
WORK, AND MUST BE DESIGNED AND
DETAILED BY ENGINEER OF RECORD

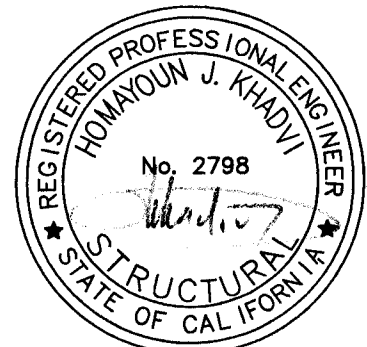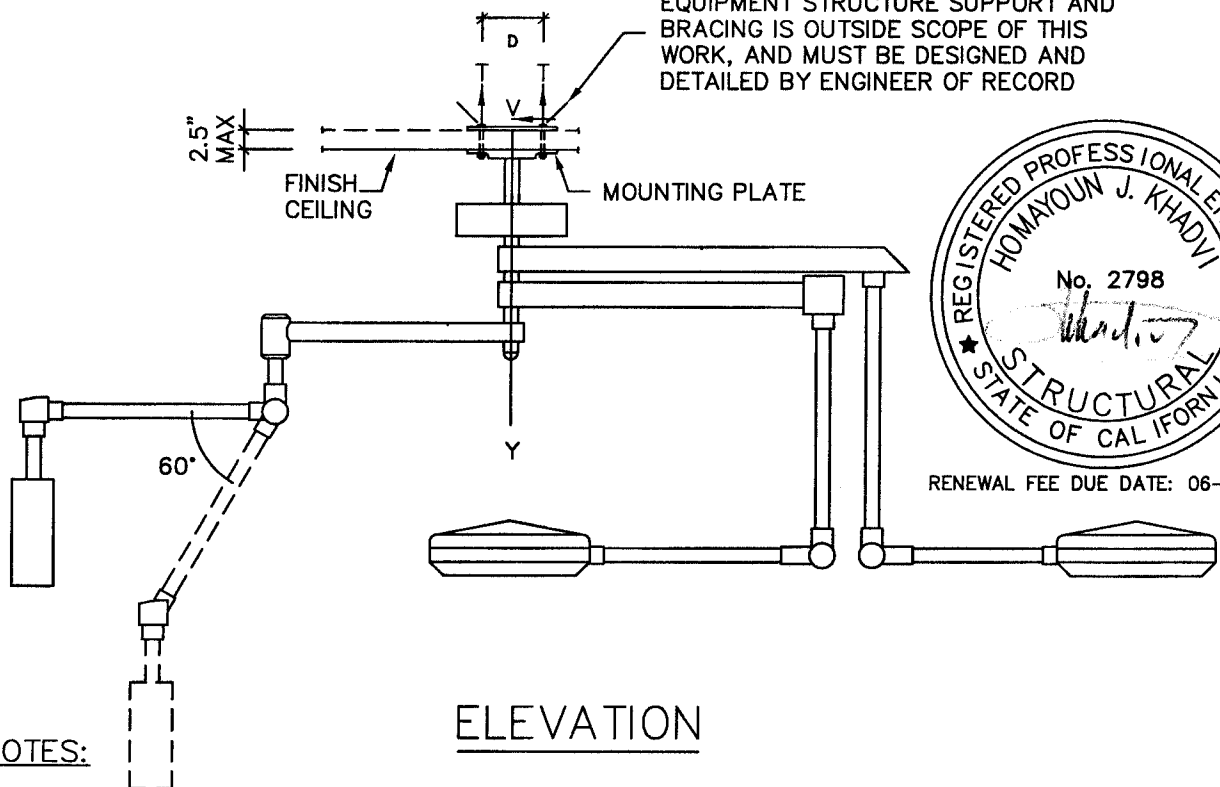

RENEWAL FEE DUE DATE: 06-30-06

ELEVATION

NOTES:

1. SCOPE OF WORK: DESIGN OF BOLTS CONNECTING MOUNTING PLATE TO STRUCTURE ONLY.
2. FORCES ARE DETERMINED PER 2001 CALIFORNIA BUILDING CODE – SECTION 1632A, (INCLUDING UP TO DATE REVISIONS) AND HAVE BEEN FACTORED TO REPRESENT WORKING DESIGN LOADS, NOT ULTIMATE
3. FORCES ARE MAXIMUMS AND OCCUR WHEN EQUIPMENT IS MOVED TO ITS MOST ECCENTRIC POSITION.
4. PROVIDE CEILING STRUCTURE DESIGNED AND DETAILS TO SUPPORT WEIGHTS AND FORCES SHOWN (BY ENGINEER OF RECORD FOR THE BUILDING)
5. ENGINEER OF RECORD TO DESIGN, DETAIL AND VERIFY STRUCTURE AND/OR EXISTING LIGHT SUPPORT TRACTS TO SUPPORT INDICATED LOADS
6. HORIZONTAL FORCES AND MOMENT MAY OCCUR IN ANY DIRECTION, ACTING AT THE TOP OF MOUNTING PLATE.

FIROUZI CONSULTING ENGINEER, INC.

SKYTRON SURGICAL PRODUCTS	DES.	SHEET 2 OF 4 SHEETS
LFSst232323	FCE JOB No.	
FOR SEISMIC ZONE (4), SOIL PROFILE (Sd) NEAR SOURCE FACTOR = 1.5	DATE: 4-6-04	

DESIGN CRITERIA:

FORMULA 32A-1: $F_p = 4.0 C_a I_p W_p$

TABLE 16A-Q : $C_a = 0.44 N_a = 0.44 \cdot 1.5 = 0.66$ (For zone 4 & S D)

TABLE 16A-K : $I_a = 1.5$ (For essential facility)

$\therefore F_p = (4.0)(0.66)(1.5)W_p = 3.96 W_p$ (For LRFD)

$F_p = 3.96 W_p / 1.4 = 2.83 W_p$ (For ASD)

FORMULA 30A-1: $E = p E_h + E_v$

$E_h = F_p$

$p = 1.0$ (FOR COMPONENT)

$E_v = (0.5) C_a I_p W_p$


$= (0.5)(0.66)(1.5)W_p = 0.5 W_p$ (For LRFD)

$= 0$ (For ASD)


SECTION 1630A.11: $E_v = (0.7) C_a I W_p$

$= (0.7)(0.66)(1.5)/1.4 = 0.5 W_p$ (For ASD) [NET UPLIFT FORCE]

LOAD COMBINATION CASE A



LOAD COMBINATION CASE B



BY COMPARISON LOAD, COMBINATION A GOVERNS

FIROUZI CONSULTING ENGINEER, INC.

SKYTRON SURGICAL PRODUCTS

DES.

SHEET

LFSst232323




FOR SEISMIC ZONE (4), SOIL PROFILE (Sd)
NEAR SOURCE FACTOR = 1.5

FCE
JOB No.

DATE: 4-6-04

3

OF 4 SHEETS

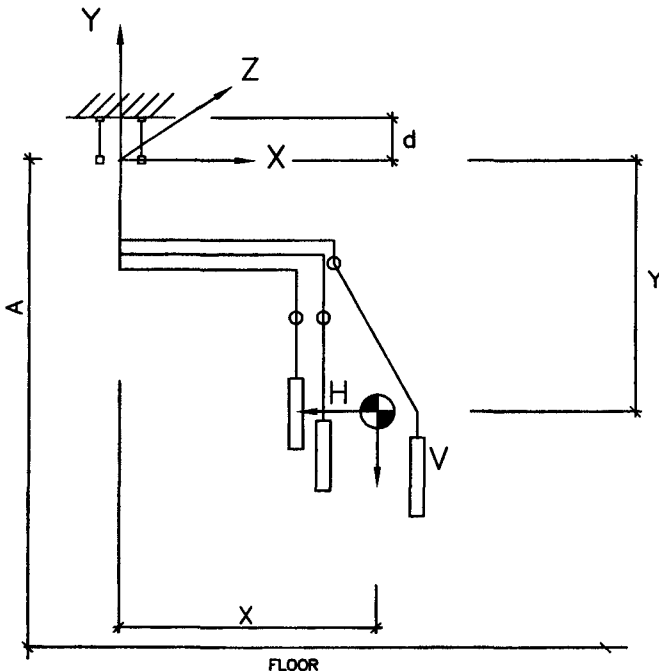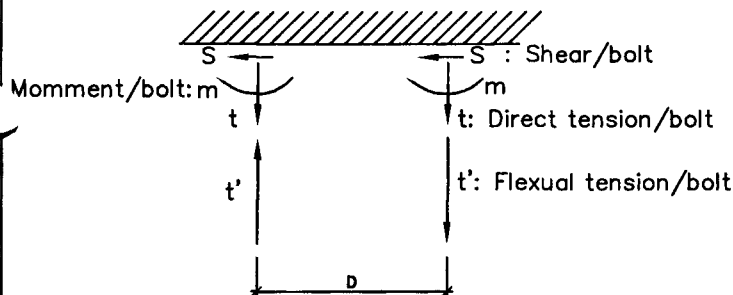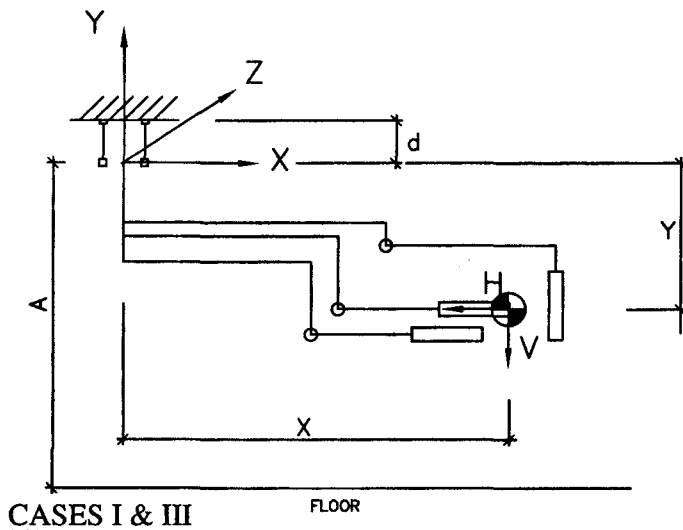

A: MAX FLOOR TO MOUNTING PLATE
DISTANCE

A = 10'-0" = 120"

Vd : Dead Load (= DL)

Ve : Vertical Seismic Load (= Ev)

He : Horizontal Seismic Load (= Eh)

CASE I (FIXTURE AT HIGH POSITION)

d = 2.5 "

D = 9.5 "

Vd = 135.0 + 100.0 + 100.0 + 100.0 = 435.0 #

Y = 120.0 - 80.0 = 40.0 "

X = (135.0 x 90.1 + 100.0 x 78.3 + 100.0 x 70.5
+ 100.0 x 62.8) / 435 = 76.6 "

Ve = 0.50 x 435.0 = 215.3 #

He = 2.83 x 435.0 = 1230.4 #

S = 1230.4 / 4.0 = 307.6 #

t = (435.0 + 215.3) / 4 = 163 #

Total Mzz = (435.0 + 215.3) x 76.6 + 1230.4 x
40.0 = 99036 "#

t' = 99036 / (9.5 x 2) = 5212 #

m = 308 x 2.5 = 769.0 "#

CASE II (FIXTURE AT LOW POSITION)

d = 2.5 "

D = 9.5 "

Vd = 435.0 #

Y = [(120.0 - 34.6) x 135.0 + (40.0 + 35.3) x
100.0 + (40.0 + 35.3) x 100.0 + (40.0 + 35.3) x
100.0] / 435.0 = 78.4 "

X = [(50.6 + 39.5 x COS(60)) x 135.0 + 43.0 x
100.0 + 35.3 x 100.0 + 27.5 x 100.0] / 435.0 =
46.2 "

Ve = 0.50 x 435.0 = 215.3 #

He = 2.83 x 435.0 = 1230.4 #

S = 1230.4 / 4.0 = 307.6 #

t = (435.0 + 215.3) / 4 = 163 #

Total Mzz = (435.0 + 215.3) x 46.2 + 1230.4 x
78.4 = 126524 "#

t' = 126524 / (9.5 x 2) = 6659 #


m = 308 x 2.5 = 769 "#

FIROUZI CONSULTING ENGINEER, INC.

SKYTRON SURGICAL PRODUCTS	DES.	SHEET 4 OF 4 SHEETS
LFSst232323	FCE JOB No.	
FOR SEISMIC ZONE (4), SOIL PROFILE (Sd) NEAR SOURCE FACTOR = 1.5	DATE: 4-6-04	

CASE III (Same As CASE I, Lateral Forces Applied Diagonally To Mounting Plate)

$$\begin{aligned}
 d &= 2.5 \text{ "} \\
 D &= 13.4 \text{ "} \\
 V_d &= 435.0 \text{ \#} \\
 Y &= 40.0 \text{ "} \\
 X &= 76.6 \text{ "} \\
 V_e &= 0.50 \times 435.0 = 215.3 \text{ \#} \\
 H_e &= 2.83 \times 435.0 = 1230.4 \text{ \#} \\
 S &= 1230.4 / 4.0 = 307.6 \text{ \#} \\
 t &= (435.0 + 215.3) / 4 = 163 \text{ \#} \\
 \text{Total } M_{zz} &= (435.0 + 215.3) \times 76.6 + 1230.4 \times 40.0 = 99036 \text{ " \#} \\
 t' &= 99036 / (13.4 \times 1) = 7371 \text{ \#} \\
 m &= 308 \times 2.5 = 769 \text{ " \#}
 \end{aligned}$$

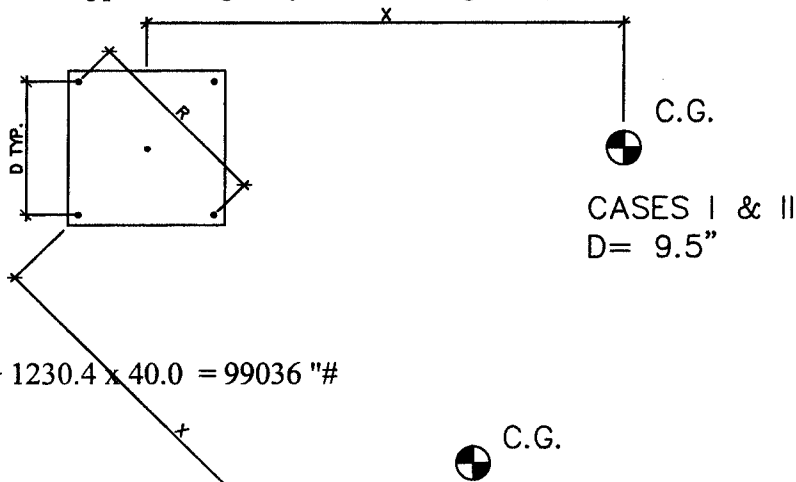

CASE IV

(Same As CASE II, Lateral Forces Applied Diagonally To Mounting Plate)

$$\begin{aligned}
 d &= 2.5 \text{ "} \\
 D &= 13.4 \text{ "} \\
 V_d &= 435.0 \text{ \#} \\
 Y &= 78.4 \text{ "} \\
 X &= 46.2 \text{ "} \\
 V_e &= 0.50 \times 435.0 = 215.3 \text{ \#} \\
 H_e &= 2.83 \times 435.0 = 1230.4 \text{ \#} \\
 S &= 1230.4 / 4.0 = 307.6 \text{ \#} \\
 t &= (435.0 + 215.3) / 4 = 163 \text{ \#} \\
 \text{Total } M_{zz} &= (435.0 + 215.3) \times 46.2 + 1230.4 \times 78.4 = 126524 \text{ " \#} \\
 t' &= 126524 / (13.4 \times 1) = 9417 \text{ \# GOVERNS} \\
 m &= 308 \times 2.5 = 769 \text{ " \#}
 \end{aligned}$$

C.G.
CASES III & IV
 $R = 9.5(2)^{0.5} = 13.4 \text{ "}$

CHECK 7/8" DIA. A490 BOLTS:

ALLOWABLE TENSION: 32500 #
ALLOWABLE SHEAR: 12600 #

$$\begin{aligned}
 S &= 3.14 \cdot d^3 / 32 = 3.14 \times (0.88)^3 / 32.0 = 0.07 \text{ "}^3 \\
 f_b &= 769.0 / 0.07 = 11699 \text{ PSI} \\
 F_b &= 0.75 \times 36000 = 27000 \text{ PSI}
 \end{aligned}$$

$$f_v / F_v + f_t / F_t + f_b / F_b = 0.02 + 0.29 + 0.43 = 0.75 < 1.0 \text{ OK}$$

USE 7/8" DIA. A490 BOLTS